



Topi-CLICK® 35 DOSE ™ Topical Dosing Dispenser

Healthcare providers and caregivers can easily verify a dose with the **NEW** graduated Topi-CLICK® 35 DoseCheck™ system.




Provides an independent check system to verify dose.



Features graduated marks at each 0.5 mL.

BOTTOM of Plunger indicates the amount of medication remaining.

Each turn/CLICK of base dispenses 0.25 mL of topical
1 CLICK = 0.25 mL
2 CLICKs = 0.50 mL

The Topi-CLICK® 35 DOSE ™ topical dosing dispenser provides the same advanced technology as the Topi-CLICK® 35 and offers **EXTRA** assurance with graduated marks so the dose starting and stopping points can be easily verified and recorded. ***Topi-CLICK® 35 DoseCheck™ initial start point should begin when the bottom of the plunger is at the 30 mL graduated mark.***

Consistent & Accurate Dose™

- Topi-CLICK® dispensers proven most accurate among others tested by *ARL
- Eliminates user-variability
- Consistent automated dosing throughout treatment
- Allows for easy recording of numerical volumes dispensed

Built-in Applicator Pad

- Reduces the risk of cross-contamination to others

CLICK-Assist™ Technology

- Clear Audible CLICKs
- Built-in Visual CLICK points
- Strong Tactile Sensations at each CLICK point

Viscosity Assurance™

- Accuracy NOT affected by varying formulations
- Accuracy NOT affected by varying bases

Made of FDA grade materials | BPA and Phthalate free | UV block and is Recyclable 

Request
*ARL PEER REVIEWED EVIDENCE at
http://doselogix.com/accuracy_study.

Topi-CLICK® 35 DOSE ™

Healthcare Provider Use Instructions

STEP 1:

Healthcare provider should begin by reading dose volume while holding the dispenser at eye level.

Record volume by reading the graduated line at the **bottom of the plunger** and then record by using the healthcare facility's preferred method of dose recording. (Figure a.)

Holding dispenser above or below eye level may cause errors in reading. Topi-CLICK® 35 DoseCheck™ initial start point should begin when the bottom of the plunger is at the 30 mL graduated mark.

Provides an independent check system to verify dose.




STEP 2:
Lift off the cap of the Topi-CLICK® dispenser by placing your thumb under the tab on the protective outer cap and pressing upward.




STEP 3:
Watch the visual indicators when rotating base. Be sure to leave the base in the registered CLICK position by aligning the base column with the tube node after each use.




STEP 4:
Turn the base to dispense the number of CLICKS or mLs specified in the instructions on the prescription label.

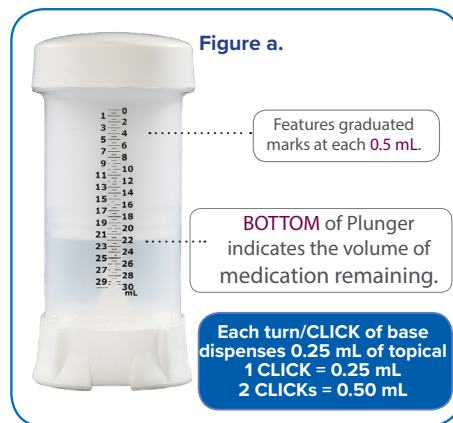


STEP 5:
Apply topical medication as directed by the physician or pharmacist. Rub the area of the skin using the **built-in applicator pad. Continue rubbing until topical is completely absorbed into the skin. IMPORTANT:** The built-in applicator lessens the risk of cross-contamination and ensures the full dose is applied to intended area.



STEP 6:
Replace cap after each dose to prevent evaporation. Be sure cap snaps on tightly.



STEP 7:
Read volume stopping point by holding dispenser at eye level and recording as indicated by your healthcare facility. (Special Note: See Figure b.)

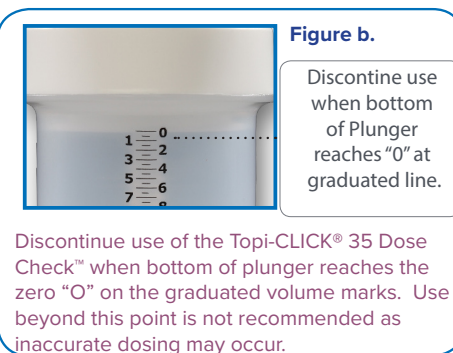

Follow instructions on prescription label before using the Topi-CLICK.®

Topi-CLICK® 35 DOSE ™ Filling Instructions

Read all information, specifications and instructions carefully before filling and dispensing Topi-CLICKs.



Note:
Before filling the Topi-CLICK® 35 DoseCheck™, apply clear tape over the graduated marks to protect rub off from oils or alcohol.



STEP 1:

Fill the Topi-CLICK® dispenser with the desired amount of topical formulations using a Topi-CLICK® Filling Station, a spatula, EMP jar, or nozzle.

STEP 2:

If needed while filling, stop periodically to tap the Topi-CLICK® on the palm of your hand, counter or Tap-n-CLICK™ to help settle the topical.

STEP 3:

Put the applicator pad (cap with a hole) on the top of the Topi-CLICK® container by aligning the inside key tabs with the slots on the top of the container tube and snap on.



STEP 4:

Prime the Topi-CLICK® by turning the base until topical is dispensed and wipe off topical.

Be sure to leave the base in the registered CLICK position by aligning the base column with the tube node: See



Registered Position

See Step 3 of the **Healthcare Provider Use Instructions**.

STEP 5:

Snap on the protective outer cap. (If the cap doesn't fit tight, it's an indication that the applicator pad in #3 is not "snapped" down all the way.)

STEP 6:


Apply center of label over the "REFILL" badge area. **Apply clear tape over the graduated marks to protect rub off from oils or alcohol.**

Topi-CLICK® 35 DoseCheck™ initial start point should begin at the 30 mL graduated mark.

For more information on dispensing amounts per CLICK see the Product Specification's at DoseLogix.com. See Healthcare Provider User Instructions for information on how to apply topical medications using Topi-CLICK. Verify formulas and weight per volume as required for compounded prescription pharmaceuticals.



Topi-CLICK® 35 DOSE™ Specifications

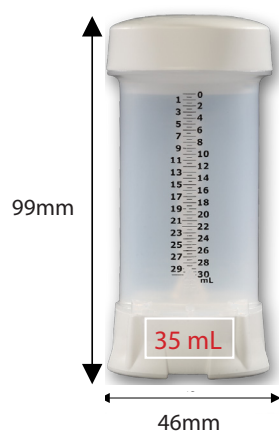

Topi-CLICK® 35 DoseCheck™: 35 mL, 0.25 mL per CLICK

DESCRIPTION: Healthcare providers and caregivers can easily verify a dose with the NEW graduated Topi-CLICK® 35 DoseCheck™ system.

The Topi-CLICK® 35 DOSE™ topical dosing dispenser provides the same advanced technology as the Topi-CLICK® 35 and offers EXTRA assurance with graduated marks so the dose starting and stopping points can be easily verified and recorded.

Topi-CLICK makes it easy to accurately measure the dose and apply topical medications to the intended area, thereby decreasing the risk of improper dosing and contamination while improving compliance and outcomes of therapy.

Topi-CLICK® 35 DoseCheck™ initial start point should begin when the bottom of the plunger is at the 30 mL graduated mark. The DoseCheck™ can hold the same amount as a Topi-CLICK® 35 but is specialized for use in settings where dose tracking is required.

FEATURES:

- Graduated marks at each 0.50 mL.
- Each CLICK or turn of the base moves the plunger approximately 0.25 mL of volume space, thereby dispensing 0.25 mL of cream on average. The most common number of CLICKs used for one dose is 2 CLICKs or 0.50 mL volume space.
- Filling: Assuming two priming CLICKs— when filling the Topi-CLICK® DoseCheck™, it is recommended to add an additional 4 mL per prescription to allow for priming, data recording marks and residual. There will normally be an additional one or two CLICKs of dispense (0.25 to 0.50 mL) after the plunger advances to the “0” mark.
- Audible, visual and tactile CLICK registrations for user recognition.
- Lower cost with simplified labeling – labels as fast and easily as a prescription bottle.
- Built-in applicator to prevent medication transference to unintended areas.
- “Refill” reminder badge helps patients to reorder in a timely manner.
- Designed to resist accidental discharge in purse, pocket or luggage.

TECHNICAL SPECIFICATIONS: Topi-CLICK® 35 DoseCheck™

Dispenser Volume:	Up to 34 mL
Delivery Volume:	30 mL (based on beginning initial start point at the 30 mL graduated mark)
Dispense per CLICK:	0.25 mL
Approximate Residual:	3.50 mL (Residual remaining after plunger reaches the “0” graduated mark.)
Approximate Priming:	0.50 mL or 2 CLICKs
Doses Provided:	The Topi-CLICK® DoseCheck™ will provide approximately 30 mL or 60 doses (at 2 CLICKs per dose or 120 CLICKs total) between the “30” and “0” graduated marks. 1 mL of cream can still be dispensed from the DoseCheck™ after reaching “0”. The 1 mL buffer space is there to ensure accurate visual dose tracking and dispensation is maintained for the patient.

- Registered FDA device, Class 1 Dispenser.
- Topi-CLICK's FDA Registration # is 3007142798 and the Device Listing Number is D309579.
- Materials compliant with FDA 21.177 code, which is the requirement for United States Pharmacopeia (USP <661>).
- Made of FDA grade materials | BPA and Phthalate free | UV block.
- Recycling Code is #5 . Visit <http://doselogix.com/recycling-your-topi-click> for more information on recycling Topi-CLICK®.

*Volumes are approximate. As required for compounded prescription pharmaceuticals dispensed in volume dispensers, verify the weight to volume conversions thoroughly. See dispensing instructions at <http://doselogix.com/downloads-how-it-works>. One time use only.

Topi-CLICK® 35 is the most accurate topical dosing dispenser among those compared in an independent study titled [Topical Metered Dosing Dispenser Performance Evaluation by Analytical Research Laboratories](http://doselogix.com/accuracy_study/). Request study at http://doselogix.com/accuracy_study/.